

# Performance evaluation of a table-top Compton camera for various detector parameters

Se Hyung Lee<sup>a</sup>, Hee Seo<sup>a</sup>, So Hyun An<sup>b</sup>, Jae Sung Lee<sup>c</sup>, Chan Hyeong Kim<sup>a,\*</sup>

<sup>a</sup>Department of Nuclear Engineering, Hanyang University, Seoul 133-791, Republic of Korea

<sup>b</sup>Korea Atomic Energy Research Institute, Daejeon 305-353, Republic of Korea

<sup>c</sup>Department of Nuclear Medicine and Interdisciplinary Program in Radiation Applied Life Science, Seoul National University, Seoul 110-744, Republic of Korea

Available online 21 March 2008

## Abstract

A prototype table-top Compton camera, composed of two small plane-type position-sensitive semiconductor detectors, is under development. The objective of this study was to find the optimal imaging conditions for the Compton camera in order to maximize its performance in terms of imaging resolution and imaging sensitivity. To that end, the performance of the Compton camera was simulated varying several detector parameters (i.e., the photon energy of the source, the geometrical configuration of the component detectors, and the interaction position resolution of the absorber detector), using the GEANT4 detector simulation toolkit. The Compton camera was found to show its highest performance for the photon energy of 364.5 keV (<sup>131</sup>I), but also showed a relatively high performance for 511 keV (<sup>18</sup>F) and 662 keV (<sup>137</sup>Cs). The Compton camera showed its highest performance also when the scatterer and absorber detectors were positioned in parallel, separated by 10 cm. Finally, it was found significantly beneficial to the imaging resolution to increase the interaction position resolution of the absorber detector to  $0.3 \times 0.3 \text{ cm}^2$  in the planar direction and to 0.5 cm in the axial direction.

© 2008 Elsevier B.V. All rights reserved.

PACS: 29.30.Kv; 29.40.Gx; 24.10.Lx

Keywords: Compton camera; Medical imaging; Position-sensitive detector; Monte Carlo; GEANT4

## 1. Introduction

The Compton camera is a very promising gamma-ray imaging device, especially in the field of nuclear medicine and molecular imaging [1–4]. The Compton camera has many advantages over conventional gamma-ray imaging devices, these advantages include 3D imaging capability from a fixed position, almost no limitation on the photon energy of the gamma sources, simultaneous multiple radioisotope tracing capability, and, in principle, high imaging resolution and sensitivity. Currently under development is a table-top Compton camera composed of small plane-type position-sensitive semiconductor detectors. The current version of the Compton camera, however, does not show sufficient imaging resolution and sensitivity for

medical imaging applications. The objective of the present study was to find the optimal imaging conditions for the table-top Compton camera in order to maximize its performance in terms of imaging resolution and imaging sensitivity. To that end, different imaging conditions were simulated using the GEANT4 detector simulation toolkit [5].

## 2. Methods

The table-top Compton camera is composed of two plane-type position-sensitive semiconductor detectors: a double-sided silicon strip detector (DSSD,  $5 \times 5 \times 0.15 \text{ cm}^3$ ,  $16 \times 16$  strips) as the scatterer detector and a 25-segmented germanium detector (25-SEG,  $5 \times 5 \times 2 \text{ cm}^3$ ,  $5 \times 5$  segments) as the absorber detector (Fig. 1) [6]. The Compton camera was simulated with the GEANT4 detector simulation toolkit. In the simulation,

\*Corresponding author. Tel.: +82 2 2220 0513; fax: +82 2 2220 4059.  
E-mail address: [chkim@hanyang.ac.kr](mailto:chkim@hanyang.ac.kr) (C.H. Kim).

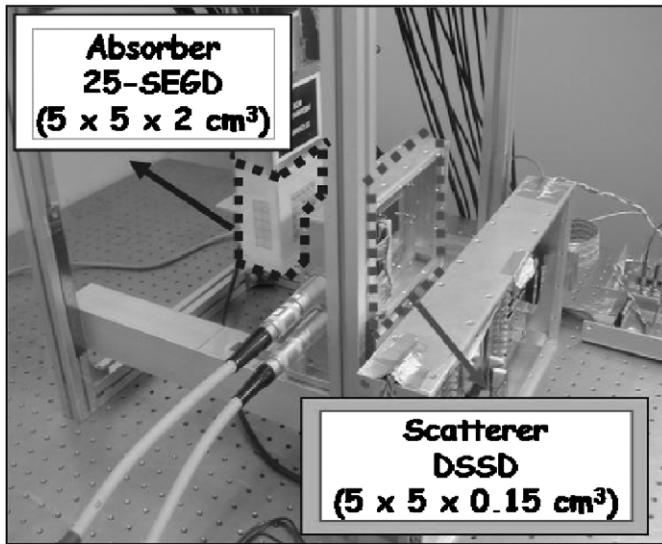


Fig. 1. Table-top Compton camera.

the energy resolution assumed 4 keV on scatterer detector and 1–2 keV on absorber detector depending on the deposited energy of the photon in the absorber detector, interaction position resolution, and energy discrimination levels of the component detectors were all modeled. Doppler energy broadening was included by implementing the Penelope physics model. To reduce computation time, the ‘exponential transform’ technique, which artificially increases the interaction probability of an incident photon in the scatterer detector, was implemented.

In this study, the performance of the table-top Compton camera was determined as a function of the photon energy of the source and the geometrical configuration of the component detectors. The performance of the Compton camera for the photon energies of 140, 364.5, 511, 662, and 1332 keV, which represent  $^{99m}\text{Tc}$ ,  $^{131}\text{I}$ ,  $^{18}\text{F}$ ,  $^{137}\text{Cs}$ , and  $^{60}\text{Co}$ , respectively, was calculated. The considered geometrical configuration variables of the component detectors were the inter-detector distances (IDDs) of 3, 6, 10, 15, and 20 cm and inter-detector angles (IDAs) of  $0^\circ$ ,  $30^\circ$ ,  $45^\circ$ ,  $60^\circ$  and  $90^\circ$ . Considering that the imaging resolution is limited mainly by poor interaction position resolution of the absorber detector [7], the Compton camera’s imaging resolution was evaluated also as a function of the interaction position resolution of the absorber detector.

### 3. Results and discussion

Fig. 2 shows the imaging sensitivity, imaging resolution, and figure-of-merit (FOM) [2] of the table-top Compton camera as a function of the photon energy of the source. The simulated photon source was a point source located 6 cm in front of the camera. The imaging sensitivity of the Compton camera is the maximum for the photon energy of 364.5 keV. For 140 keV, the imaging sensitivity is very low, mainly because most of the photon energies deposited in the scatterer detector are very small and thus easily

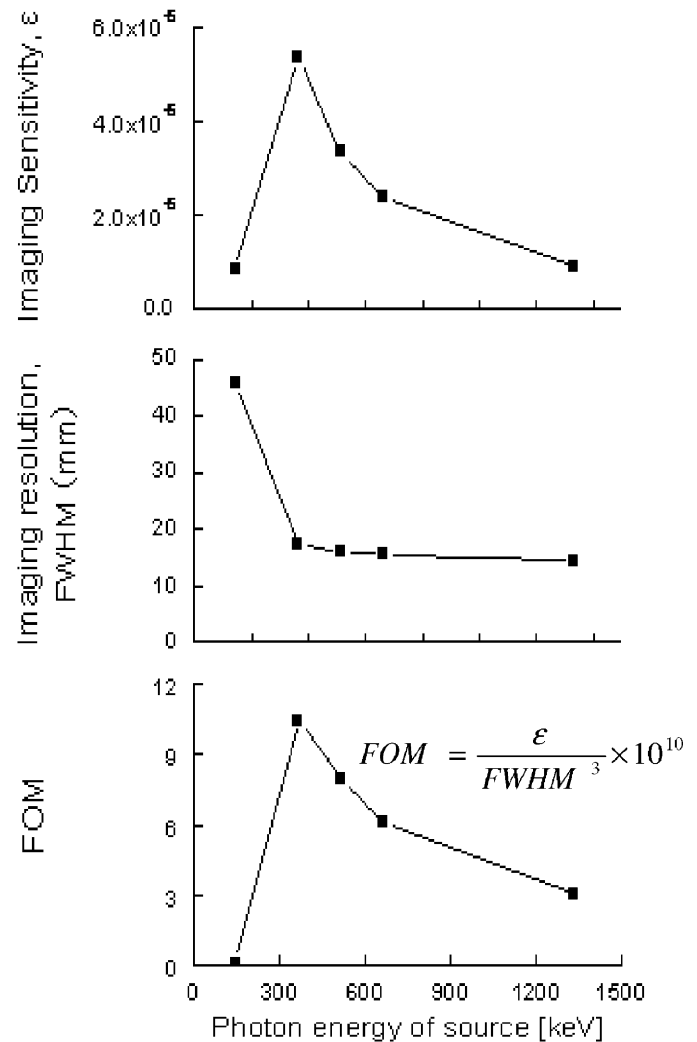


Fig. 2. Variation of the imaging sensitivity, imaging resolution, and figure-of-merit (FOM) of table-top Compton camera as a function of photon energy of source.

discriminated by the energy discrimination level of the scatterer detector (20 keV). Above 364.5 keV, the imaging sensitivity decreases as the photon energy increases, due simply to the decline of the interaction probability for higher-energy photons. Fig. 2 also shows that the imaging resolution of the Compton camera does not significantly improve for photon energies greater than 364.5 keV, mainly because the effect of Doppler energy broadening is significant only when the photon energy is very small [8]. The slight increase of the imaging resolution over 364.5 keV seems related to the energy resolution characteristics of the component detectors. Overall, the table-top Compton camera shows its highest performance (highest FOM) for the photon energy of 364.5 keV, but also shows relatively high performances for 511 and 662 keV.

Fig. 3 shows the performance of the table-top Compton camera as functions of the IDD and IDA for an  $^{18}\text{F}$  point source 6 cm in front of the Compton camera. With increasing IDD, the effect of the interaction position resolution of the component detectors on the imaging

Download English Version:

<https://daneshyari.com/en/article/1828448>

Download Persian Version:

<https://daneshyari.com/article/1828448>

[Daneshyari.com](https://daneshyari.com)