



28th International Symposium on Superconductivity, ISS 2015, November 16-18, 2015, Tokyo, Japan

R&D Progress of HTS Magnet Project for Ultrahigh-field MRI

Taizo Tosaka^{a,*}, Hiroshi Miyazaki^a, Sadanori Iwai^a, Yasumi Otani^a, Masahiko Takahashi^a, Kenji Tasaki^a, Shunji Nomura^a, Tsutomu Kurusu^a, Hiroshi Ueda^{b,d}, So Noguchi^{c,d}, Atsushi Ishiyama^d, Shinichi Urayama^e, Hidenao Fukuyama^e

^aToshiba corporation, 2-4 Tsurumi, Yokohama 230-0045, Japan

^bOsaka University, 10-1Mihogaoka, Ibaraki, Osaka 565-0047, Japan

^cHokkaido University, Kita 14 Nishi 9, Kita, Sapporo 060-0814, Japan

^dWaseda University, 3-4-1 Ohkubo, Shinjyuku, Tokyo 169-8555, Japan

^eKyoto University, 54 Shogoinkawaharacho, Sakyo, Kyoto 606-8507, Japan

Abstract

An R&D project on high-temperature superconducting (HTS) magnets using rare-earth $\text{Ba}_2\text{Cu}_3\text{O}_7$ (REBCO) wires was started in 2013. The project objective is to investigate the feasibility of adapting REBCO magnets to ultrahigh field (UHF) magnetic resonance imaging (MRI) systems. REBCO wires are promising components for UHF-MRI magnets because of their superior superconducting and mechanical properties, which make them smaller and lighter than conventional ones. Moreover, REBCO magnets can be cooled by the conduction-cooling method, making liquid helium unnecessary. In the past two years, some test coils and model magnets have been fabricated and tested. This year is the final year of the project. The goals of the project are: (1) to generate a 9.4 T magnetic field with a small test coil, (2) to generate a homogeneous magnetic field in a 200 mm diameter spherical volume with a 1.5 T model magnet, and (3) to perform imaging with the 1.5 T model magnet. In this paper, the progress of this R&D is described. The knowledge gained through these R&D results will be reflected in the design of 9.4 T MRI magnets for brain and whole body imaging.

© 2016 Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

Peer-review under responsibility of the ISS 2015 Program Committee

Keywords: MRI; Magnet; Ultra-high field; REBCO; HTS coil; Screening current

1. Introduction

The nuclear magnetic resonance (NMR) signals from, for example, carbon, phosphorous, nitrogen and oxygen may become easier to detect in high magnetic fields above 7 T. Therefore, novel diagnostic equipment based on ultrahigh-field (UHF) magnetic resonance imaging (MRI) is expected [2]. Rare-earth $\text{Ba}_2\text{Cu}_3\text{O}_7$ (REBCO) wires are promising components for UHF-MRI magnets because REBCO wires have high critical current density in high magnetic fields and high mechanical strength in the longitudinal direction, whose features make REBCO magnets smaller and lighter than low-temperature superconducting (LTS) magnets. In addition, since REBCO magnets can be cooled by using the conduction-cooling method, liquid helium is not required, in contrast to LTS magnets, in which a huge amount of liquid helium is consumed at initial cooling and cooling after quenching. Against this background, an R&D project on REBCO

* Corresponding author. Tel.: +81-45-510-6695; fax: +81-45-500-1973.

E-mail address: taizo.tosaka@toshiba.co.jp

magnets for UHF-MRI systems was started in 2013 [2] [3]. In the past two years, some test coils and model magnets have been fabricated and tested to identify the difficulties and problems faced and to establish basic magnet technologies. This paper describes the progress of this R&D project.

2. Project goals

The overall project objective is to investigate the feasibility of adapting REBCO magnets to UHF-MRI systems. The project term is three years, and this year is the final year. The project goals, to be achieved by March 2016, are as follows:

- To demonstrate the generation of a 9.4 T magnetic field with a 10 T test coil
- To demonstrate the generation of a homogeneous magnetic field in a 200 mm diameter spherical volume (DSV) with a 1.5 T model magnet
- To perform imaging with the 1.5 T model magnet

A magnetic field of 9.52 T has already been demonstrated with a 10 T coil, shown in Fig. 1 (a), under conduction-cooling conditions. The 10 T test coil was composed of twenty-two single pancake coils, with an inner diameter of 50 mm, an outer diameter of 129 mm, and a height of 104 mm. Each single pancake coil was wound with a 4 mm-wide and 0.1 mm-thick REBCO wire, and was impregnated with epoxy resin. The 1.5 T model magnet shown in Fig. 1(b) is currently being fabricated. It has three sets of split coils, split coils #1, #2 and #3 shown in Fig. 1(b), which are made of stacked single pancake coils. The number of single pancake coils in split coils #1, #2 and #3 are a pair of six, a pair of ten and a pair of fourteen, respectively.

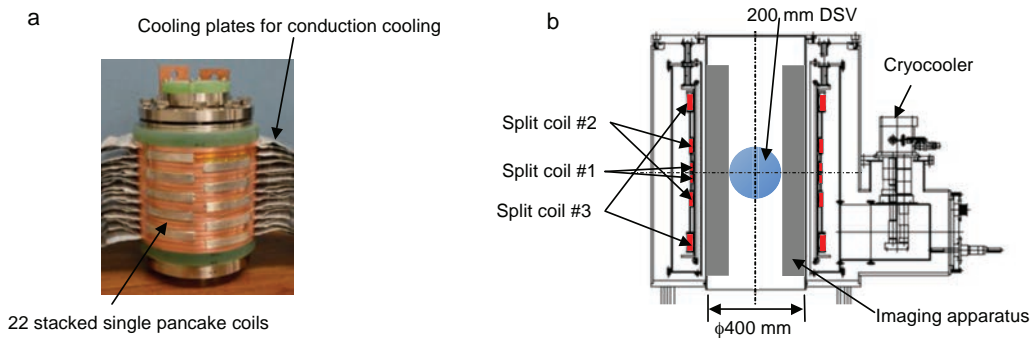


Fig. 1. (a) Photograph of 10 T test coil ; (b) Cross-section of 1.5 T model magnet.

3. R&D progress of technical issues

In this project, some test coils and model magnets have been fabricated and tested to investigate the challenging technical issues faced in realizing a UHF-MRI system. R&D progress of the most important technical issues, that is, generation of a homogeneous and stable magnetic field and coil protection, are described below

3.1. Homogeneous magnetic field

There are some peculiar causes of irregular magnetic fields when using REBCO magnets. These are mainly based on the tape shape of REBCO wires, including that of a filament. In this subsection, the influence of screening current fields and dimensional errors is described. The influence of screening current fields was investigated with the 10 T coil stated above. The measured screening current fields, for example, 0.4 T in the maximum case, with hysteresis behavior were well described by a simulation program developed in previous studies[4] [5]. The influence of the screening current fields of a whole body MRI magnet was calculated to be less than 100 ppm using the same simulation program. Therefore, the irregular magnetic fields due to the screening current seem to be predictable at the level of 100 ppm.

On the other hand, the influence of the dimensional errors was investigated with a 1 T model magnet shown in Fig. 2 [6]. The 1 T model magnet has two pairs of coil units, which consist of a pair of two single pancake coils and a pair of four single pancake coils. The room temperature bore is 200 mm in diameter, and homogeneous region is designed to be

Download English Version:

<https://daneshyari.com/en/article/1873179>

Download Persian Version:

<https://daneshyari.com/article/1873179>

[Daneshyari.com](https://daneshyari.com)