



Applied Radiation and Isotopes 64 (2006) 1238-1241

Applied Radiation and Isotopes

www.elsevier.com/locate/apradiso

Standardization of ²⁴¹Am solution

Marina F. Koskinas*, Eliezer A. Silva, Ione M. Yamazaki, Mauro S. Dias

Instituto de Pesquisas Energéticas e Nucleares (IPEN-CNEN/SP), Centro do Reator de Pesquisas-CRPq, C.P. 11049, Pinheiros, 05422-970-São Paulo-SP, Brazil

Abstract

The standardization of 241 Am solution has been undertaken using a $4\pi\beta-\gamma$ coincidence system. The 4π proportional counter used for alpha detection has a 0.1 mm thick Al window in the outside wall in order to minimize γ -ray attenuation. The extrapolation technique was applied to determine the activity of the solution. The variation of alpha efficiency has been made using external absorbers and by the electronic discrimination. The results from the two methods were compared and are in agreement within the experimental uncertainty. © 2006 Elsevier Ltd. All rights reserved.

Keywords: Activity; 241 Am; Coincidence system; Disintegration rate

1. Introduction

Am-241 decays with half-life of 432.6 y (Chechev and Kuzmenko, 2004), emitting alpha particles populating the excited levels of $^{237}{\rm Np}$ which emit gamma-rays to achieve the stable level (Fig. 1). $^{241}{\rm Am}$ is one of the most important radionuclides used as standard source for α and γ spectrometers. To γ spectrometers, its importance is due to the low gamma energy (59.54 keV) emitted with 35.78% intensity, which is in a region lacking in standards. For this reason $^{241}{\rm Am}$ has been selected by the CCRI(II) (Comité Consultative pour les Etalons de Mesures des Rayonnements Ionisants II) for an international comparison.

The LMN, Nuclear Metrology Laboratory from IPEN has participated in this comparison in collaboration with the Laboratório Nacional de Metrologia das Radiações Ionizantes (LNMRI) from Rio de Janeiro.

The standardization of 241 Am presented in this paper was undertaken in a 4π (PC)-NaI(Tl) coincidence system. The 4π proportional counter used for alpha detection has a 0.1 mm thick Al window in the outside wall in order to minimize γ -ray attenuation. The extrapolation technique was applied in order to determine the activity of the solution (Baerg, 1967). The alpha efficiency was changed by two different methods: the first made use of external

absorbers of Collodion films with $20\,\mu g\,cm^{-2}$ gold coated, placed over and under the sources; the second was by electronic discrimination, changing the alpha spectrum threshold. The events were registered by a method developed by the LMN that makes use of a time to amplitude converter (TAC) associated with a Multichannel Analyser (Lavras et al., 2001).

2. Experimental method

2.1. Source preparation

The ²⁴¹Am solution was sent by the Bureau International des Poids et Mesures (BIPM) to the LNMRI, in Rio de Janeiro, and a fraction forwarded to LMN in São Paulo. The sources to be measured were prepared by dropping known aliquots of the solution on a 20 μg cm⁻² thick Collodion film. This film had been previously coated with a 10 μg cm⁻² gold layer in order to render the film conductive. A seeding agent (CYASTAT SM) was used to improve the deposit uniformity and the sources were dried in a desiccator. The mass determination has been performed using the pycnometer technique (Campion, 1975).

2.2. $4\pi\beta-\gamma$ Coincidence method

A 4π proportional counter filled with P-10 gas and operated at 0.1 MPa was used for alpha detection. Its

^{*}Corresponding author. Tel.: +551138169176; fax: +551138169188. E-mail address: koskinas@net.ipen.br (M.F. Koskinas).

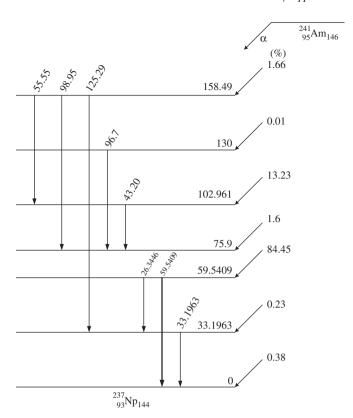


Fig. 1. Simplified decay scheme of ²⁴¹Am. All energies are in keV.

outside wall (with a 0.1 mm thick Al window) was coupled to the crystal scintillator, in order to minimize γ -ray attenuation. The gamma detector was a $58 \, \text{mm} \times 58 \, \text{mm}$ NaI(Tl), instead of the usual $76 \, \text{mm} \times 76 \, \text{mm}$, in order to reduce the background in the $59 \, \text{keV}$ region selected for the gamma channel window.

The formulae applied to the coincidence measurement is given by the well-known relationship (Baerg, 1967):

$$\frac{N_{\alpha}N_{\gamma}}{N_{c}} = N_{0} \left\{ 1 + \left(\frac{1 - \varepsilon_{\alpha}}{\varepsilon_{\alpha}} \right) \left(\frac{\alpha \varepsilon_{ec} + \varepsilon_{\alpha \gamma}}{1 + \alpha} \right) \right\},\,$$

where N_0 is the disintegration rate, N_{α} the proportional counter counting rate, N_{γ} the γ -channel counting rate, N_c the coincidence rate, ε_{α} the proportional counter efficiency for alpha particles, $\varepsilon_{\alpha\gamma}$ the proportional counter efficiency for γ -rays, ε_{ec} the proportional counter efficiency for conversion electron, α the total conversion coefficient.

The observed counting rates N_{α} and N_{γ} were corrected for background, dead time and decay in the usual way. The coincidence rate N_c was corrected for dead time and accidental coincidences using the Cox-Isham formalism (Cox and Isham, 1977) adapted by Smith (1978).

The electronic diagram system used is presented in Fig. 2. In the TAC method, the signals after selection in the SCA Timing are sent to two gates and delay generators that yield the start and stop information to the TAC. A typical spectrum obtained in the multichannel analyzer is shown in Fig. 3. In this figure the first peak is due to the alpha counts without coincidences, the middle peak corresponds to the coincidences counts and the last peak

is due to the gamma counts without coincidences. The total alpha counts are given by the integration of two first peaks, the total gamma counts are given by the integration of the second and third peaks and the coincidence counts are given by the integration of the middle peak. For the dead time correction, the ratio live time/real time obtained from the multi channel analyzer was used. The correction for accidentals was performed by subtracting the expected accidental counting rate given by $N_{\rm ACC} = \tau_{\rm r} N_{\alpha} N_{\gamma}$, where

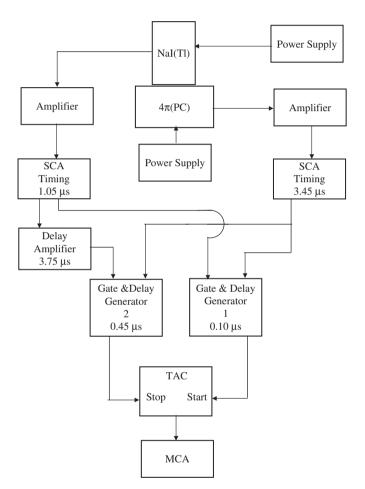


Fig. 2. Schematic diagram of the electronic system.

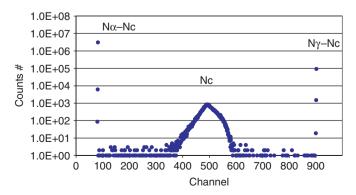


Fig. 3. Typical TAC spectrum.

Download English Version:

https://daneshyari.com/en/article/1879859

Download Persian Version:

https://daneshyari.com/article/1879859

<u>Daneshyari.com</u>