

SHORT COMMUNICATION

Haemozoin Detection in Mouse Liver Histology Using Simple Polarized Light Microscope

DWI RAMADHANI*, SITI NURHAYATI, TUR RAHARDJO

*Center for Technology of Radiation Safety and Metrology, National Nuclear Energy Agency of Indonesia
Jalan Lebak Bulus Raya No. 49, Kotak Pos 7043, Jakarta 12070, Indonesia*

Received February 25, 2013/Accepted September 6, 2013

The presence of malarial pigment (haemozoin) due to *Plasmodium* infection is a common histopathological effect in mouse liver. Previous research showed that by using a polarized light microscope, researchers were better able to detect haemozoin in mouse liver histology section. Thus, the aim of this research was to compare the haemozoin area observed by a conventional vs. simple polarized light microscope by using image processing analysis. A total of 40 images produced from both conventional light microscope and simple polarized light microscope were collected. All images were analyzed using ImageJ 1.47 software to measure the haemozoin areas. Our results showed that non birefringent haemozoin and birefringent haemozoin area was significantly different. This was because when using conventional light microscope the brown area that contained images of non birefringent haemozoin images also contained Kupffer cells which appeared as the same brown color as haemozoin. In contrast, haemozoin gave bright effect and can be easily differentiated with Kupffer cells in the birefringent haemozoin images. This study concluded that haemozoin detection in mouse liver histology using a simple polarized light microscope was more accurate compared to that of conventional light microscope.

Keywords: haemozoin, liver histology, mouse, microscope, polarization

INTRODUCTION

Malaria is a serious global disease and a leading cause of morbidity and mortality in tropical and subtropical countries. It affects between 350 and 500 million people worldwide and causes more than one million deaths each year (Syaifudin *et al.* 2011). Malaria is caused by protozoan parasites of the genus *Plasmodium* (Hisaeda *et al.* 2005) and its common histopathological effect due to *Plasmodium* infection is the presence of haemozoin in the liver (Baheti *et al.* 2003). Haemozoin is a heme polymer produced by the parasite as a result of hemoglobin breakdown inside the red blood cells (RBC) of the host. The lysis of red blood cells during infection results in release of merozoites with this heme pigment, which are phagocytized by circulating monocytes, neutrophils and resident macrophages (Sullivan & Meshnick 1996; Egan 2003). The amount of haemozoin in tissues increases over the duration of infection, therefore the amount of pigment correlates with the chronicity of the lesion (Silva *et al.* 2011). As a result of haemozoin

accumulation, liver histology is reveals congestion with brown or black pigmentation (Baheti *et al.* 2003).

Examination of haemozoin in liver histology is usually manually identified under microscope. It is commonly observed in association with late stage parasitic infection or as an indicator of previous (including treated) infection. Because it contains a birefringent (doubly refracting) substance, haemozoin is highly visible when viewed using crossed polarized light (Lawrence & Olson 1986). The haemozoin in human placental histological specimens using polarizing microscope was more sensitive than conventional light microscope (Romagosa *et al.* 2004). However, the haemozoin detection using polarized light microscope can produce false results. This is because dust and dirt on the slide may produce a birefringence similar to that of haemozoin. However such false positive results can be avoided by double checking the pigment containing cells for parasites by using light microscopy (Romagosa *et al.* 2004).

Maude *et al.* (2009) devised a simple method for adapting a conventional light microscope for polarized light microscopy. They used a pair of gray or black polarizing sunglasses and a small

*Corresponding author. Phone: +62-21-7513906/7659511,
Fax: +62-21-7657950, E-mail: dhani02@btan.go.id

additional piece of polarizing material that had been cut out of from a plastic polarizing lens or a polarizing test strip. The researchers placed a black polarizing sunglass on the top of light source of microscope and a piece of polarizing material placed on the top of thick blood smear slide from a patient with severe malaria. This apparatus was able to can successfully identify haemozoin inside the slide (Maude *et al.* 2009). Here in this study, we adapted those techniques using a conventional light microscope for polarized light microscope to detect haemozoin area in the mouse (*Mus musculus* sp.) liver section histology. The aim of this research was to compare the measurements of haemozoin area obtained using a conventional light microscope vs. a simple polarized light microscope by using image processing analysis.

MATERIALS AND METHODS

Polarized Light Microscope. A Nikon Biophot microscope was used as a conventional light microscope. The equipments required for adapting Nikon Biophot to become a polarized light microscope were a linear polarizing sheet (45 x 35 mm) (Polar Pro) and commercial circular polarizing filter (CPL) 58 mm (Hoya Pro1) for Digital Single Lens Reflex (DSLR) Camera. The CPL filter 58 mm was placed on the top of the microscope light source and the linear polarizing sheet was placed on the top of liver histology slide. The slides were examined under 40x objective lens with maximum brightness (Figure 1). The CPL filter was rotated in a clockwise direction until it reached the position where the object appeared to be most dark. The difference between light and dark was approximately in 45° of rotation. The angle at which the object appears darkest was noted (Kramer *et al.* 2001).

Mouse (*Mus musculus* sp.) Liver Histology. Mouse (*Mus musculus* sp.) liver histology slides

were made in 7 µm thickness using hematoxylin eosin (HE) stain and were obtained from the Nuclear Biomedical Laboratory in the Center for Technology of Radiation Safety and Metrology, National Nuclear Energy Agency of Indonesia. Mice were inoculated with the irradiated *Plasmodium berghei* of an ANKA strain at a dose of 150 Gy and were kept for 24 days before proceeding to liver histological study.

Image Acquisition. A Nikon Biophot microscope attached to Nikon D3000 digital single lens reflects (DSLR) camera system was used to capture the images of the blood smear slides. Images were captured at a resolution of 1936 x 1296 pixel and saved as JPEG files. The first image was captured using the adapted polarized light microscope, whereas the second image was captured using the same setting but after removal of the linear polarizing sheet and CPL filter. A total of 20 images were collected using simple polarized and conventional light microscope.

Image Analysis. A macro program was developed in ImageJ 1.47 for measuring the birefringent haemozoin area in mouse liver histology. The algorithm of macro program can be divided into the following several sequential steps (Figure 2). The first step was to split the images channels into green, blue and red channels. The second step was to invert the green channel image to detect the haemozoin area using thresholding methods. The last step was to measure the haemozoin area and determine the outlined haemozoin area in the images. The haemozoin area in images captured using the conventional light microscope was measured by using an ImageJ 1.47 plugin previously developed (unpublished data). To obtain the measurement of the areas presented in micrometer (µm) the Set Scale command in ImageJ must be employed. First an image of a microscope stage micrometer under the same microscope magnification that

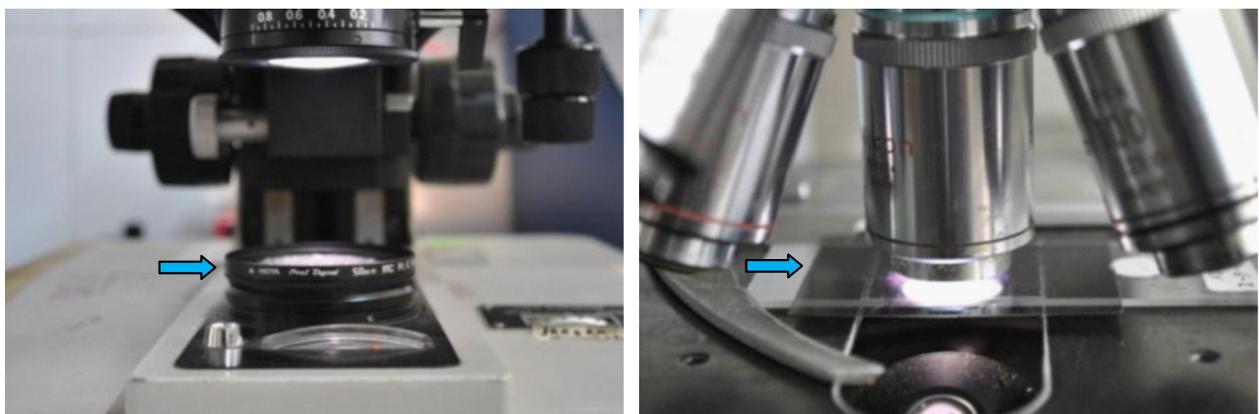


Figure 1. CPL filter 58 mm on top of the microscope light source (blue arrow) (left) and a linear polarizing sheet on the top of a liver histology slide (blue arrow) (right).

Download English Version:

<https://daneshyari.com/en/article/2085870>

Download Persian Version:

<https://daneshyari.com/article/2085870>

[Daneshyari.com](https://daneshyari.com)