



## Case Report

## Cardiac erosion after catheter closure of atrial septal defect: Septal malalignment may be a novel risk factor for erosion



Yasufumi Kijima (MD, PhD)<sup>a</sup>, Teiji Akagi (MD, PhD, FJCC)<sup>b,\*</sup>, Koji Nakagawa (MD, PhD)<sup>a</sup>,  
Worakan Promphan (MD)<sup>c</sup>, Norihisa Toh (MD, PhD)<sup>a</sup>,  
Kazufumi Nakamura (MD, PhD, FJCC)<sup>a</sup>, Shunji Sano (MD, PhD, FJCC)<sup>b</sup>,  
Hiroshi Ito (MD, PhD, FJCC)<sup>a</sup>

<sup>a</sup> Department of Cardiovascular Medicine, Okayama University Hospital, Okayama, Japan

<sup>b</sup> Division of Cardiac Intensive Care Unit, Okayama University Hospital, Okayama, Japan

<sup>c</sup> Department of Pediatrics, Prince of Songkla University, Hat Yai, Thailand

## ARTICLE INFO

## Article history:

Received 22 August 2013

Received in revised form

22 November 2013

Accepted 9 December 2013

## Keywords:

Atrial septal defect

Erosion

Complication

Pediatric interventions

## ABSTRACT

Pericardial tamponade occurred 3 days after the catheter closure of an atrial septal defect (ASD) using Amplatzer Septal Occluder (St. Jude Medical, St. Paul, MN, USA). Before the closure, two-dimensional and real-time three-dimensional transesophageal echocardiography demonstrated a deficient aortic rim and atrial septal malalignment. Perforation of the right atrium toward the non-coronary sinus of the aortic root was confirmed at the emergent surgery. Cardiac erosion is one of the most catastrophic complications in ASD patients undergoing catheter closure with Amplatzer Septal Occluder. Hence, several risk factors for this complication are discussed and identified. Oversized device deployment and a deficient aortic rim are accepted factors potentially causing cardiac erosion. Besides, atrial septal malalignment, which is a morphological characteristic of ASD, may be a novel risk factor for cardiac erosion.

**<Learning objective:** Cardiac erosion is a potentially lethal complication when catheter closure of atrial septal defects using Amplatzer Septal Occluder (St. Jude Medical, St. Paul, MN, USA) is provided to the patients. However, mechanisms of this complication remain to be completely elucidated. Atrial septal malalignment may be one of the novel risk factors for this catastrophic complication.>

© 2013 Japanese College of Cardiology. Published by Elsevier Ltd. All rights reserved.

## Introduction

Catheter closure of atrial septal defect (ASD) is an accepted highly successful alternative to surgical repair [1,2]. In catheter closure of ASD using Amplatzer Septal Occluder (St. Jude Medical, St. Paul, MN, USA), a cardiac erosion followed by a pericardial tamponade is an infrequent but potentially lethal complication and is difficult to anticipate its occurrence before the device deployment [3,4].

## Case report

A 44-year-old woman with dyspnea on exertion was referred to our institution for catheter closure of an ASD. Transthoracic echocardiography (TTE) demonstrated a secundum ASD with


a significant left-to-right shunt with right ventricular dilatation. Transesophageal echocardiography (TEE) revealed a maximal defect diameter of 21 mm with adequate rims surrounding the defects except for a deficient aortic rim (Fig. 1A). Morphological characteristics including atrial septal malalignment were visualized using two-dimensional TEE (Fig. 1B and C) and real-time three-dimensional TEE (Fig. 1D). Written informed consent was obtained from the patient prior to the procedure.

Catheter closure was performed under general anesthesia. Pulmonary to systemic flow ratio was 3.14. Balloon-sizing with stop flow technique demonstrated a 25 mm stretched diameter. A 26-mm Amplatzer Septal Occluder device was deployed in a stable and a proper position without any procedural complications. Images from TEE demonstrated the device properly deployed against the atrial septum and a residual shunt between the device and the aortic root (Fig. 2A–C).


Three days after the procedure, the patient developed pericardial tamponade. The patient was transferred to emergent surgery. Surgical findings demonstrated perforation in the right atrium

\* Corresponding author at: Division of Cardiac Intensive Care Unit, Okayama University Hospital, 2-5-1 Shikata-cho, Kita-ku, Okayama 7008558, Japan.  
Tel.: +81 86 235 7357; fax: +81 86 235 7683.

E-mail address: [t-akagi@cc.okayama-u.ac.jp](mailto:t-akagi@cc.okayama-u.ac.jp) (T. Akagi).

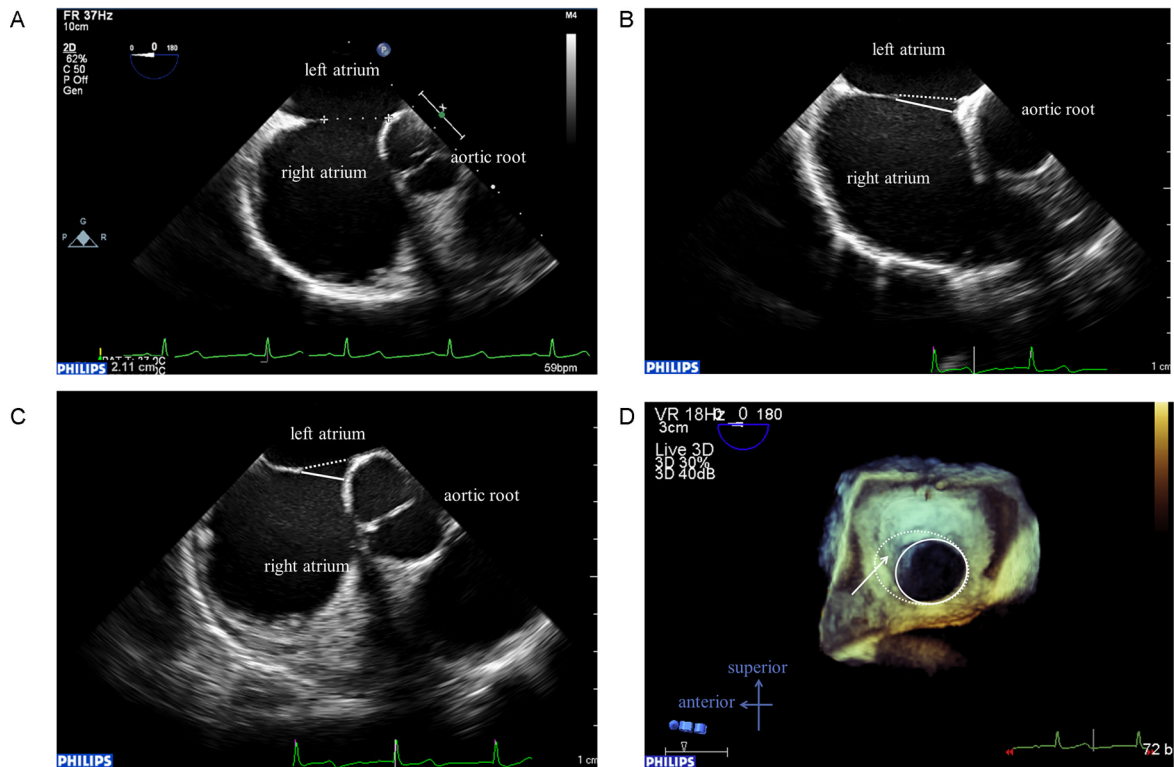

**Fig. 1.** Transesophageal echocardiography (TEE) images of atrial septal defect before the procedure. (A) Two-dimensional 0° TEE image shows that the maximal defect diameter of septum primum was 21 mm. (B and C) Two-dimensional 30° TEE image shows that the defect surface of the septum primum (dotted-line) is different from that of the septum secundum (solid-line). Images of the defect on end systolic phase (B) and early diastolic phase (C). (D) Three-dimensional TEE image shows an en face view from the left atrium. Arrow indicates the deficient aortic rim. Surface of the left atrial side consists of septum primum (dotted-line) while surface of the right atrial side consists of septum secundum (solid-line). These two surfaces construct the morphological characteristic of the malaligned atrial septum.

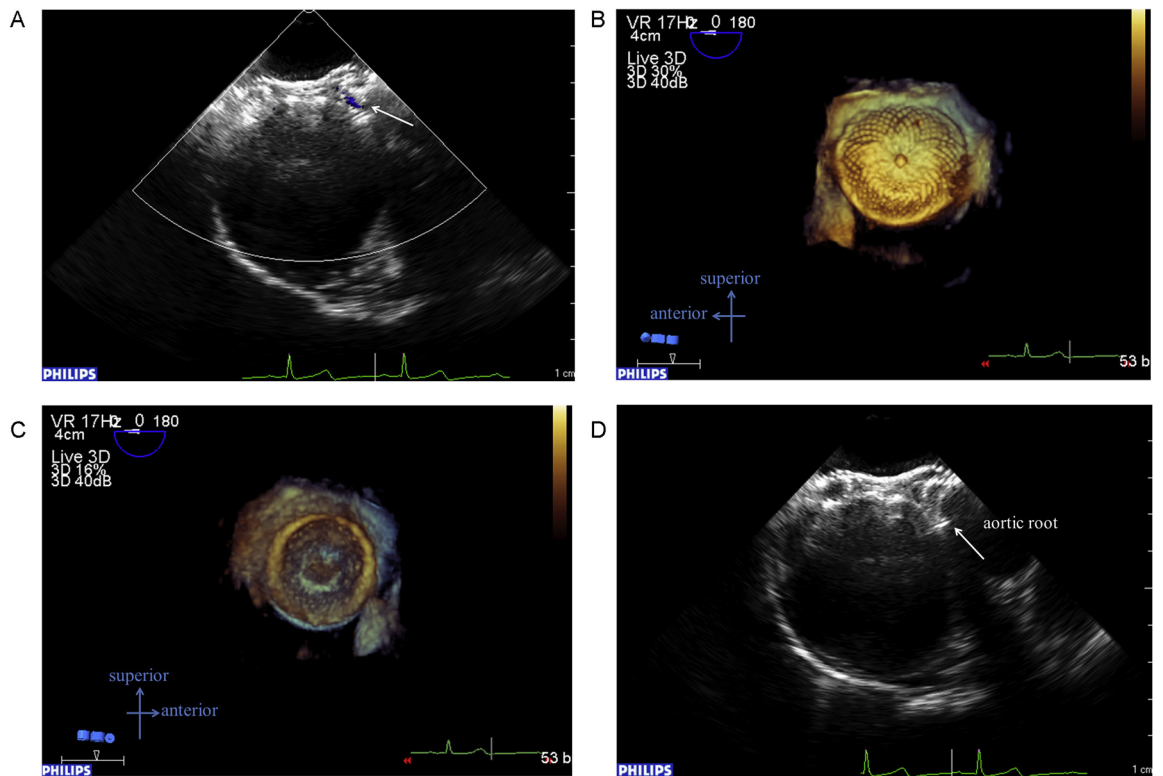

**Fig. 2.** Deployed images of the device. (A) The image shows the device deployed in an appropriate position against the atrial septum. A small residual shunt from the aortic side is demonstrated in a color Doppler image (arrow). (B and C) Three-dimensional transesophageal echocardiography (TEE) shows the device properly deployed against the atrial septum visualized in views from the left atrium (B) and from the right atrium (C). (D) TEE image of the deployed device. Right atrial side of the device is tightly impinging on the aortic root (arrow).

Download English Version:

<https://daneshyari.com/en/article/5984749>

Download Persian Version:

<https://daneshyari.com/article/5984749>

[Daneshyari.com](https://daneshyari.com)