

Clinical paper

Tracheal rapid ultrasound saline test (T.R.U.S.T.) for confirming correct endotracheal tube depth in children[☆]

Mark O. Tessaro^{a,*}, Evan P. Salant^b, Alexander C. Arroyo^a, Lawrence E. Haines^a, Eitan Dickman^a

^a Department of Emergency Medicine, Division of Emergency Ultrasound, Maimonides Medical Center, 4802 10th Ave, Brooklyn, NY 11219, United States

^b Department of Anesthesiology, Division of Emergency Ultrasound, Maimonides Medical Center, 4802 10th Ave, Brooklyn, NY 11219, United States

ARTICLE INFO

Article history:

Received 24 April 2014

Received in revised form 8 August 2014

Accepted 24 August 2014

Keywords:

Diagnostic accuracy

Ultrasound

Intubation

Endotracheal tube

Pediatrics

Endobronchial intubation

ABSTRACT

Objective: We evaluated the accuracy of tracheal ultrasonography of a saline-inflated endotracheal tube (ETT) cuff for confirming correct ETT insertion depth.

Methods: We performed a prospective feasibility study of children undergoing endotracheal intubation for surgery. Tracheal ultrasonography at the suprasternal notch was performed during transient endobronchial intubation and inflation of the cuff with saline, and with the ETT at a correct endotracheal position. Ultrasound videos were recorded at both positions, which were confirmed by fiberoptic bronchoscopy. These videos were shown to two independent blinded reviewers, who determined the presence or absence of a saline-inflated cuff. The primary outcome was accuracy of tracheal ultrasonography for appropriate ETT insertion depth.

Results: Forty-two patients were enrolled. For correct endotracheal versus endobronchial positioning, pooled results from the reviewers revealed a sensitivity of 98.8% (95% CI = 90–100%), a specificity of 96.4% (95% CI = 87–100%), a PPV of 96.5% (95% CI = 87–100%), a NPV of 98.8% (95% CI = 89–100%), a positive likelihood ratio of 32 (95% CI = 6–185), and a negative likelihood ratio of 0.015 (95% CI = 0.004–0.2). Agreement between reviewers was high (kappa co-efficient = 0.93; 95% CI = 0.86 to 1). The mean duration of the ultrasound exam was 4.0 s (range 1.0–15.0 s).

Conclusions: Sonographic visualization of a saline-inflated ETT cuff at the suprasternal notch is an accurate and rapid method for confirming correct ETT insertion depth in children.

© 2015 Published by Elsevier Ireland Ltd.

1. Introduction

Inadvertent endobronchial ETT placement occurs in up to 30% of pediatric emergency intubations¹. Unrecognized endobronchial intubation increases the risk of hypoxia and barotrauma that can cause neurologic injury and death^{2–4}. Critically ill pediatric patients are at particular risk from these complications, as children have higher oxygen consumption rates than adults and their indication for emergency intubation is often respiratory failure.

Chest x-ray is the most commonly used test to confirm ETT depth, but has numerous drawbacks. It may take approximately 20 min to generate a result^{5,6}, exposing patients with inadvertent endobronchial intubations to a dangerously long period with a

misplaced ETT. It also requires lifting of the patient to place the x-ray film, which risks dislodging the ETT.

In the hands of appropriately trained providers, bedside ultrasonography of the anterior neck can accurately distinguish between tracheal or esophageal intubation^{5,7–13}, but has only been able to detect ETT tip depth in newborns^{14,15}. Indirect ultrasound surrogates of correct ETT insertion depth (bilateral lung sliding and diaphragm movement) are inferior to chest radiography^{6,16}, and are not useful in cases of pneumothorax, subcutaneous emphysema, pleural scarring, pleural effusion, pulmonary malignancies, or endotracheal tube obstruction⁶.

An ETT cuff located at the level of the suprasternal notch correlates to correct depth of ETT insertion¹⁷. While a cuff filled with air cannot be sonographically distinguished from the surrounding air-filled trachea, prior reports in adult patients¹⁸ and cadavers¹⁹ showed that ultrasonography at the suprasternal notch can visualize a saline-inflated ETT cuff. The use of saline in an ETT cuff is a well-established and safe practice^{20–31}, but no studies have explored the use of sonography on a saline-inflated ETT cuff to

[☆] A Spanish translated version of the summary of this article appears as Appendix in the final online version at <http://dx.doi.org/10.1016/j.resuscitation.2014.08.033>.

* Corresponding author.

E-mail address: oliver.tessaro@gmail.com (M.O. Tessaro).

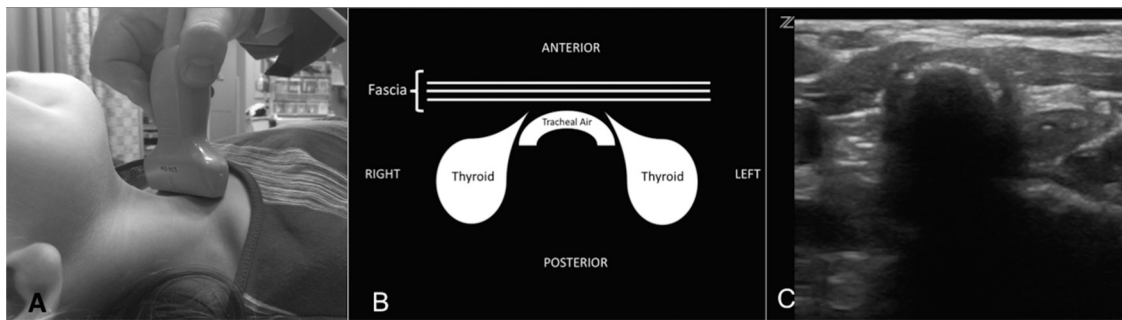


Fig. 1. Ultrasound technique. (A) Transducer position. The probe is held perpendicular to the anterior neck at the level of the suprasternal notch. The probe marker is towards the patient's right. (B) Diagram of airway structures as they appear on ultrasound imaging at this location. Tracheal air causes acoustic shadowing that eliminates visualization of deeper tissues. (C) Sonographic image corresponding to (B).

rule out endobronchial intubation, and no studies have included children.

Bedside ultrasonography of a saline-inflated ETT cuff would be an ideal intubation depth verification test as it involves no radiation, requires no patient repositioning, gives an instantaneous result, and can be repeated as frequently as needed. It could potentially improve patient safety during pediatric intubation by rapid and accurate detection of endobronchial intubation.

We sought to determine whether the use of a saline-inflated ETT cuff would allow rapid and accurate ultrasonographic confirmation of correct ETT insertion depth in pediatric patients undergoing general anesthesia.

2. Methods

2.1. Study design and setting

This was a prospective feasibility study enrolling a convenience sample of pediatric patients undergoing general anesthesia requiring endotracheal intubation in the operating room of our institution's ambulatory surgery center. Approval for the study was obtained from the Institutional Review Board of Maimonides Medical Center (study number 2013-02-19).

2.2. Selection of participants

Families of patients aged 3 months to 18 years who were scheduled for procedures involving endotracheal intubation and were ASA class 1 or 2 were approached in the pre-operative area of the ambulatory surgery center. Patients were excluded if they had developmental delay (due to inability to provide assent), an anticipated difficult intubation, a congenital airway anomaly, a nasogastric tube, or guardians that did not read or speak English. Informed consent was obtained from parents, and patient assent was obtained in children 7 years of age or older.

2.3. Study protocol

The anesthesiologist performed a validated pediatric intubation technique involving transient right mainstem endobronchial intubation^{32–35}, and the ETT cuff was inflated with saline in the right mainstem bronchus as well as in the trachea, with these positions confirmed by the gold standard of fiberoptic bronchoscopy. An investigator recorded ultrasound video clips with the transducer positioned on the anterior neck at the sternal notch prior to the intubation, at the time of endobronchial intubation, and when the ETT tip was positioned in the trachea.

Sonograms were performed by a pediatric emergency medicine ultrasonography fellow. Prior to the start of the study this fellow performed airway ultrasonography of intubated patients as

part of his clinical practice, and after performing 10 of these sonographic examinations, the fellow developed proficiency in recognizing the sonographic appearance of a saline-inflated cuff at the distal portion of the ETT. We used an ultrasound system (z.one ultra sp; Zonare Medical Systems, Mountain View, CA) with a 5–10 MHz linear transducer. The transducer was placed in a transverse orientation perpendicular to the anterior neck at the level of the sternal notch (Fig. 1).

Patients were nasally or orally intubated by an anesthesiologist using standard polyvinyl chloride ETTs with a high-volume, low-pressure cuff (Hi-Lo ETT, Mallinckrodt, Dublin, Ireland). A fiberoptic bronchoscope was introduced through the ETT and advanced to just within the right mainstem bronchus. The ETT was introduced into the mainstem bronchus over the bronchoscope, which was then removed. The ETT cuff was inflated with saline, with a manometer used to ensure cuff pressure did not rise above 35 cm H₂O. The ETT was left in the endobronchial position for no longer than 6 s, and was then withdrawn until the sonographer noted the appearance of the saline-inflated cuff at the level of the sternal notch, and the time from the initiation of ETT withdrawal until cuff visualization was recorded. Fiberoptic bronchoscopy was then repeated to establish whether the ETT tip was in a correct endotracheal position, using markings on the bronchoscope to measure the distance from the carina to the tip of the ETT. A fiberoptic bronchoscope with an insertion diameter of 2.2 mm (Olympus LF-P, Center Valley, PA) was used with ETTs with inner diameters of 3.5–5.0 mm, while a scope with an insertion diameter of 4.0 mm (Olympus LF-2) was used with ETTs with inner diameters of 5.5–6.5 mm and a scope with an insertion diameter of 5.2 mm (Olympus LF-TP) was used with ETTs with inner diameters of 7.0–8.0 mm.

The sonographer recorded 6 s video clips at three time points: prior to intubation (unintubated control), during cuff inflation at the endobronchial position, and at the time of cuff visualization. To reduce bias on the part of the sonographer (who was not blinded to the ETT tip position), the video clips from all patients were pooled together and their order randomized using the random sequence generator at www.random.org, and then presented to two blinded reviewers, who independently rated each clip for the presence or absence of a saline-inflated cuff. These reviewers were both board certified emergency physicians who had completed a one year emergency ultrasound fellowship and who each had more than 5 years experience in bedside sonography. Prior to rating the video clips, these reviewers underwent a 30 min lecture on airway ultrasound in intubated patients.

2.4. Outcomes

The primary outcome was the diagnostic accuracy of ultrasonography of a saline-inflated ETT cuff in confirming correct ETT position and excluding endobronchial intubation.

Download English Version:

<https://daneshyari.com/en/article/5997941>

Download Persian Version:

<https://daneshyari.com/article/5997941>

[Daneshyari.com](https://daneshyari.com)