



Contents lists available at ScienceDirect

Journal of Biomechanics

journal homepage: [www.elsevier.com/locate/jbiomech](http://www.elsevier.com/locate/jbiomech)  
[www.JBiomech.com](http://www.JBiomech.com)

Short communication

## Automated objective robot-assisted assessment of wrist passive ranges of motion

Mingming Zhang<sup>a,d,\*</sup>, Sihui Zhang<sup>a</sup>, Andrew McDaid<sup>a</sup>, Claire Davies<sup>b</sup>, Sheng Q. Xie<sup>c</sup><sup>a</sup> Department of Mechanical Engineering, The University of Auckland, Auckland, New Zealand<sup>b</sup> Department of Mechanical and Materials Engineering, Queen's University, Kingston, Canada<sup>c</sup> School of Electronic and Electrical Engineering, The University of Leeds, Leeds, United Kingdom<sup>d</sup> State Key Lab of Digital Manufacturing Equipment & Technology, Huazhong University of Science and Technology, Wuhan, China

## ARTICLE INFO

## Article history:

Accepted 3 March 2018

Available online xxxx

## Keywords:

Robotic

Assessment technique

Wrist

Passive range of motion

## ABSTRACT

The measurement of wrist passive ranges of motion (ROMs) can provide insight into improvements and allow for effective monitoring during a rehabilitation program. Compared with conventional methods, this study proposed a new robotic assessment technique for measuring passive ROMs of the wrist. The robotic system has a reconfigurable handle structure that allows for multi-dimensional applications of wrist motions. The assessment reliability of this robotic system was analysed on 11 subjects for measuring wrist extension/flexion and radial/ulnar deviation. Preliminary data demonstrated its potential with intraclass correlation coefficient (ICC<sub>2,1</sub>) all greater than 0.857 and standard error of measurement (SEM) less than 3.38°. Future work will focus on the standardization of the assessment protocol of this robotic system for assessment purposes, paving the way for its clinical application.

© 2018 Published by Elsevier Ltd.

### 1. Introduction

Although the human wrist is a biomechanical marvel when it is intact and functioning, orthopedic or neurological impairments inevitably cause dysfunction to its motion (Skirven et al., 2011). Over the past few decades, a variety of robot-assisted rehabilitation techniques have been developed to restore wrist/hand motor function. Krebs et al. (2007) integrated a wrist robotic device into the shoulder-and-elbow MIT-MANUS. Initial clinical results demonstrated the efficacy of this robot in providing continuous passive motion, strength, sensory, and sensorimotor training for the wrist. Squeri et al. (2014) developed a haptic robot to quantify motor impairment and assist wrist articular movements. The proposed adaptive control strategy showed great potential in maximizing the recovery of the wrist ranges of motion (ROMs). An important feature of robot-assisted therapy is that exercises should be tailored to specific impairments (Sanguineti et al., 2009). Passive ROM is of high clinical importance in therapy and assessment of musculoskeletal disorders. Typically in robot rehabilitation an initial active ROM target is set so that subjects can easily achieve the goal, and that ROM is progressively modified over

the course of the entire protocol. However, these existing rehabilitation systems have not been implemented with assessment of passive wrist ROMs, nor has any method been validated to reliably assess passive ROMs.

This study proposes a new robot-assisted assessment technique for measuring passive ROMs of the human wrist. The reliability of this method for measuring wrist extension/flexion (E/F) and radial/ulnar deviation (RD/UD) is analysed. To the best of the authors' knowledge, this is the first example of robot-assisted automation of assessing passive wrist ROMs based on predefined joint torque values. The reconfigurable robotic design is also a novel device which allows continuous posture adjustment of the handle.

### 2. Methods

#### 2.1. Participants

Eleven healthy subjects (six males: Age  $26.17 \pm 4.22$  years, Height  $173.83 \pm 7.28$  cm, Weight  $79.83 \pm 10.03$  kg, and five females: Age  $26.40 \pm 5.98$  years, Height  $164.20 \pm 3.49$  cm, Weight  $55.30 \pm 5.72$  kg) volunteered to participate in this study. The study was approved by the University of Auckland, Human Participants Ethics Committee (019707) and consents were obtained from all participants.

\* Corresponding author at: Department of Mechanical, Auckland University, 20 Symonds Street, Auckland 1142, New Zealand.

E-mail address: [mzha130@aucklanduni.ac.nz](mailto:mzha130@aucklanduni.ac.nz) (M. Zhang).

## 2.2. Instrumentation

The proposed assessment technique is implemented using a reconfigurable wrist rehabilitation robot and an adaptive passive assessment strategy, as in Fig. 1. The robot mechanically consists of a handle, a handle holder, the base, and the forearm holder with straps. The handle can be rotated along the handle holder for arbitrary posture adjustment. To follow convention (Horger, 1990), the motion measurement of wrist E/F is achieved by setting 0° of the handle (horizontal), and that of RD/UD by adjusting the handle to 90° (vertical).

Its electronic control system consists of a flat brushless motor (EC 90, Maxon), a magnetic rotary sensor (AS5048A, AMS), and a static torque sensor (JNNT-1, Zhongwan), which allows the implementation of adaptive passive assessment technique. The robot reverses when real-time human-robot interaction torque triggers a predefined value of wrist passive torque. Data of the angular position of the human wrist are collected from the built-in magnetic rotary sensor.

## 2.3. Procedures

Subjects sat on a height-adjustable chair with the forearm strapped and hand grasping the handle. The wrist joint was visually adjusted to approximate the rotational axis of the wrist robot, with fingers holding the handle for assessment exercises. The device was set with two configurations: 0° for wrist E/F and 90° for wrist RD/UD. The predefined wrist passive torque was set with two grades: 2.5/3.5 Nm for males and 2/2.5 Nm for females. These values were set using experience from pilot trials, and in clinical practice can be predefined by therapist based on a specific subject and his/her pathology. Thus there are a total of four measures (APA-0-L, APA-0-H, APA-90-L, and APA-90-H), where APA means adaptive passive assessment, 0 or 90 is the position of the handle, L or H refers to the level of torque limit (Low level: 2 Nm for females and 2.5 Nm for males, High level: 2.5 Nm for females and 3.5 Nm for males). For each measure, each participant was required to repeat 12 cycles of the passive assessment movement. This device was driven to work in a constant low-velocity environment (5°/s) to mimic clinical wrist rehabilitation exercises.

## 2.4. Statistics

Intraclass correlation coefficient (ICC) was used to examine the test–retest reliability of the four measures. Absolute reliability was determined by calculating the standard error of measurement

(SEM) and smallest real difference (SRD) with 95% confidence interval, as in Eqs (1) and (2) (Weir, 2005), where standard deviation (SD) is the mean SDs of all measurements. SEM % and SRD % were also calculated to facilitate the comparability with other studies. In this study, ICC<sub>2,1</sub> was selected for data analysis with two-way random, absolute agreement, 95% confidence interval.

$$SEM = SD\sqrt{(1 - ICC)} \quad (1)$$

$$SRD = SEM * 1.96 * \sqrt{2} \quad (2)$$

## 3. Results

Each participant conducted 12 cycles of passive assessment movement for each measure. The maximum and minimum joint angle values can be extracted for each cycle. To minimize the effects from random factors, such as active engagement with the robot from human users, each data set finally includes 10 elements by removing the maximum and minimum values. To facilitate data analysis in SPSS, Table 1 presents the mean and SD of measurements over all participants for each measure and each cycle, where wrist ROM values do not vary in a predictable way with the measurement cycle. It is assumed that exercises with 12 cycles of measurements are not enough for an increase of wrist ROM, and the influence of removing maximum and minimum values is negligible.

Table 2 summarizes the statistical results of the test-retest reliability of the selected four measures, where all ICC<sub>2,1</sub> values are greater than 0.857 and SEM values are less than 3.38°. Munro's correlation description (Munro, 2004) is used to interpret ICC values as high reliability of APA-0-H-F and APA-90-H-UD. The reliability of all others is excellent with ICC<sub>2,1</sub> no less than 0.9.

## 4. Discussion and conclusion

To achieve adaptive robotic protocols, assessment is normally required to tune controllers based on training performance or joint capacity. Squeri et al. (2014) explored an adaptation law by increasing task difficulty as a subject succeeds in completing a task, and assessed wrist ROMs by the use of the Fugl-Meyer assessment technique (Gladstone et al., 2002). While this robotic system showed promise in increasing wrist ROMs and decreasing its spasticity, it did not allow for automatic detection of the joint ROMs. In contrast, the proposed robot-assisted technique in this study can conduct automatic assessment of human wrist ROMs. Even though

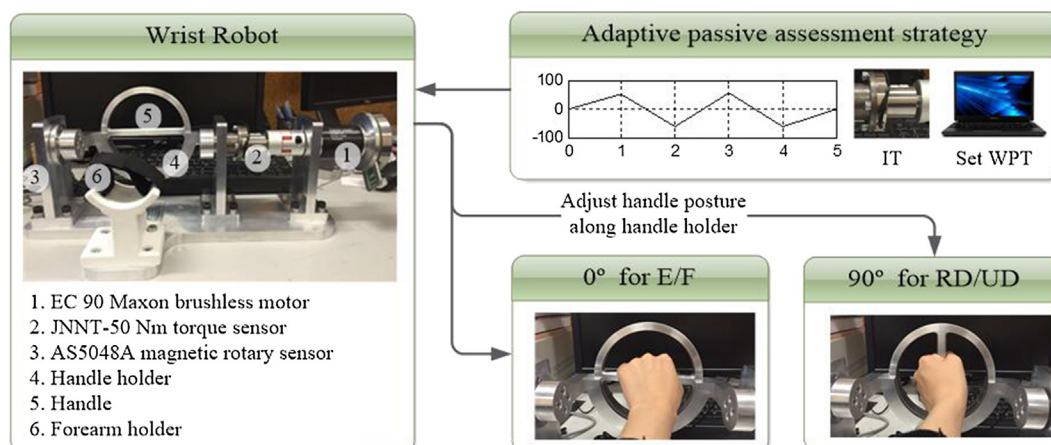


Fig. 1. A reconfigurable wrist rehabilitation robot. (IT: Interaction torque; WPT: Wrist passive torque; E/F: Extension/flexion; RD/UD: Radial/ulnar deviation).

Download English Version:

<https://daneshyari.com/en/article/7236201>

Download Persian Version:

<https://daneshyari.com/article/7236201>

[Daneshyari.com](https://daneshyari.com)