



Precision timing measurements for high energy photons



Dustin Anderson^{a,*}, Artur Apreysan^a, Adi Bornheim^a, Javier Duarte^a, Harvey Newman^a,
Cristian Pena^a, Anatoly Ronzhin^b, Maria Spiropulu^a, Jason Trevor^a, Si Xie^a, Ren-Yuan Zhu^a

^a California Institute of Technology, 1200 E California Blvd, Pasadena, CA 91125, USA

^b Fermi National Accelerator Laboratory, P.O. Box 500, Batavia, IL 60510, USA

ARTICLE INFO

Available online 21 November 2014

Keywords:

Precision timing

Calorimetry

High energy physics

Picosecond

ABSTRACT

Particle colliders operating at high luminosities present challenging environments for high energy physics event reconstruction and analysis. We discuss how timing information, with a precision on the order of 10 ps, can aid in the reconstruction of physics events under such conditions. We present calorimeter based timing measurements from test beam experiments in which we explore the ultimate timing precision achievable for high energy photons or electrons of 10 GeV and above. Using a prototype calorimeter consisting of a $1.7 \times 1.7 \times 1.7 \text{ cm}^3$ lutetium–yttrium oxyortho-silicate (LYSO) crystal cube, read out by micro-channel plate photomultipliers, we demonstrate a time resolution of $33.5 \pm 2.1 \text{ ps}$ for an incoming beam energy of 32 GeV. In a second measurement, using a $2.5 \times 2.5 \times 20 \text{ cm}^3$ LYSO crystal placed perpendicularly to the electron beam, we achieve a time resolution of $59 \pm 11 \text{ ps}$ using a beam energy of 4 GeV. We also present timing measurements made using a shashlik-style calorimeter cell made of LYSO and tungsten plates, and demonstrate that the apparatus achieves a time resolution of $54 \pm 5 \text{ ps}$ for an incoming beam energy of 32 GeV.

© 2014 Elsevier B.V. All rights reserved.

1. Introduction

Current and future high energy particle colliders are capable of providing instantaneous luminosities of $10^{34} \text{ cm}^{-2} \text{ s}^{-1}$ and above [1]. The high center of mass energy, the large number of simultaneous collisions of beam particles in the experiments, and the very high repetition rates of the collision events pose huge challenges for physics event reconstruction. They result in extremely high particle fluxes, causing high occupancies in the particle detectors operating at these machines. To reconstruct the physics events, the detectors must make as much information as possible available on the final state particles.

Precise timing of particles from high energy beam collisions is one promising method for successfully reconstructing physics events. Measuring particle time of flight (TOF) with a precision on the order of 10 ps would allow one to associate individual particles to primary collision vertices with a precision of about 1 cm or less, allowing spurious particles to be rejected from the physics events of interest.

In high energy hadron collisions, about one-third of the typical particle flux is detected as photons stemming from neutral meson decays, identified by means of their interaction with scintillating

material in the detector. Due to the abundance of photons in hadron collisions, it is viable to consider calorimeter based TOF detectors, in which the energies and TOF of incoming high energy photons are measured simultaneously via scintillators interfaced with fast photodetectors. Calorimeter based options for time measurement could provide an alternative to dedicated TOF devices on particle detectors, simplifying detector design.

One candidate scintillator for a calorimeter based TOF detector is cerium-doped lutetium–yttrium oxyortho-silicate (LYSO). LYSO crystals are desirable for timing applications because of their fast rise time ($< 72 \text{ ps}$ [2]) and high scintillation light yield (in excess of 30,000 photons/MeV [3]). Their radiation hardness also makes them ideal for use in high energy physics experiments.

The time resolution attained by a crystal calorimeter is influenced by a number of independent factors [4] (see Fig. 1). In addition to contributions from the DAQ and the photodetector(s), the resolution is affected by jitter in the scintillation process and in the optical transit time of scintillation photons in the crystal. For high energy photons incident on the calorimeter, variation in the conversion depth also impacts the total time resolution.

To test the viability of a calorimeter based TOF detector, one should isolate the effects of these different factors and determine the contribution of each one to the time resolution. In this study we aim to investigate the effects of the scintillation process and the optical transit time on the TOF resolution. To best isolate these effects, we use beams of high energy electrons (which do not need

* Corresponding author.

E-mail address: djanders@caltech.edu (D. Anderson).

to convert before beginning the scintillation process) instead of photons, and make use of the fastest photodetectors and readout electronics available.

2. Experimental setup

2.1. TOF resolution using a $1.7 \times 1.7 \times 1.7 \text{ cm}^3$ LYSO crystal

Measurements of electron TOF resolution using LYSO crystals were carried out at the Fermilab Test Beam Facility (FTBF) using beams of electrons with energies varying between 4 GeV and 32 GeV. The experimental setup is shown in Fig. 2 and schematically in Fig. 3. The electron beam impinges upon a small LYSO cube ($1.7 \times 1.7 \times 1.7 \text{ cm}^3$) that is coupled optically to a Photek 240 micro-channel plate PMT (MCP-PMT). Lead bricks are placed in front of the MCP-PMT to shield it from direct hits by the electron beam. A second Photek 240 device is placed upstream to provide a time reference. A Cherenkov detector, further upstream, discriminates between electrons and other, unwanted particles in the incoming beam. The three MCP-PMTs and the Cherenkov detector are connected to a DRS4 digitizer unit [5] for readout. A small piece of scintillator, coupled to two XP-2020 PMTs and placed in the beamline, is used as an external trigger for the DRS4 unit. Coincidence between the two XP-2020 PMTs is required in order for an event to be recorded.

The DRS4 unit has a sampling rate of 5 GHz. To determine the unit's intrinsic time resolution, light pulses from a picosecond laser are directed onto an MCP-PMT, whose output is split and sent to two different DRS4 input channels. The time difference between the signals recorded on the two channels is measured for many incident laser pulses, and the RMS of the distribution of time differences is taken as a measure of the intrinsic DRS4 time resolution. This method yields a time resolution for the DRS4 unit of about 5 ps. The time

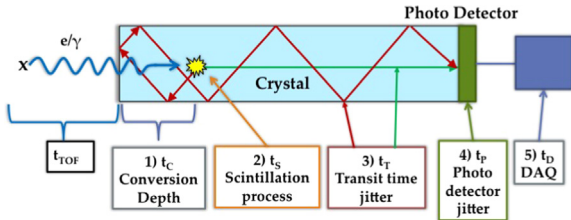


Fig. 1. Schematic showing various contributions to the resolution obtained when measuring time using crystal scintillation light [4].

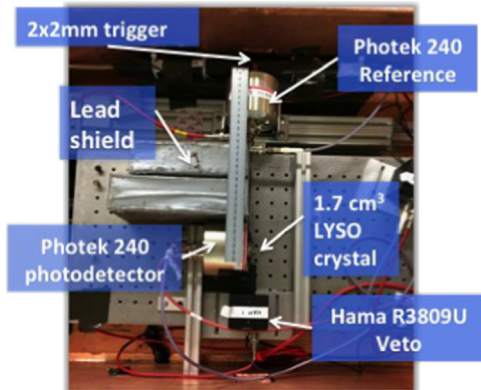


Fig. 2. Photo of the setup used to measure electron time of flight with a $1.7 \times 1.7 \times 1.7 \text{ cm}^3$ LYSO crystal interfaced with an MCP-PMT photodetector and read out using a DRS4 digitizer unit. The beam arrives from the top edge of the picture. A Hamamatsu R3809U MCP-PMT is placed downstream of the setup in order to tag beam particles not fully absorbed by the LYSO crystal, but it is not used to reject events.

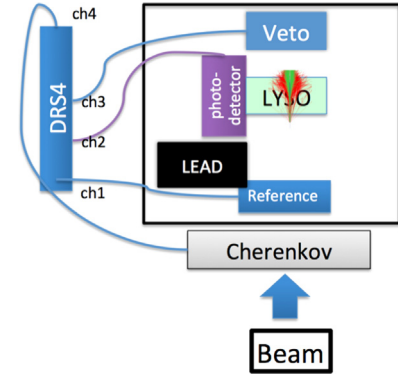


Fig. 3. Diagram of the setup used to measure electron time of flight with a $1.7 \times 1.7 \times 1.7 \text{ cm}^3$ LYSO crystal interfaced with an MCP-PMT photodetector and read out using a DRS4 digitizer unit.

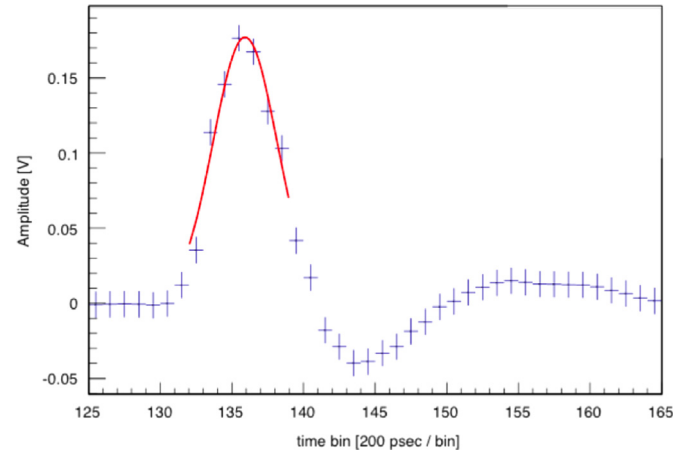


Fig. 4. Digitized pulse from the reference MCP-PMT, coarse-grained to show the pulse structure. A Gaussian fit to the pulse is used to extract a reference time stamp for the TOF measurement.

resolution of the reference time detector and DRS4 combined is approximately 20 ps [6].

In events that pass the DRS4 external trigger and are not rejected by the Cherenkov detector, the TOF between the reference MCP-PMT and the MCP-PMT attached to the LYSO crystal is measured. The time is extracted from the reference MCP-PMT using a Gaussian fit to the digitized pulse shape (see Fig. 4). The time is extracted from the MCP-PMT attached to the LYSO crystal using a constant-fraction fit to the rising edge of the scintillation pulse (see Fig. 5). The difference between these two numbers is taken as the TOF. The TOF distribution for all selected events is fit with a Gaussian, whose RMS is taken as the TOF resolution.

2.2. TOF resolution using a $2.5 \times 2.5 \times 20 \text{ cm}^3$ LYSO crystal

In a second measurement, the TOF resolution is measured using a large $2.5 \times 2.5 \times 20 \text{ cm}^3$ LYSO crystal placed perpendicularly to the incoming electron beam. A picture of this setup is shown in Fig. 6. Photek 240 MCP-PMTs are optically coupled to the ends of the crystal, and a Hamamatsu R3809U MCP-PMT is placed downstream as a time reference. The three MCP-PMTs are read out using the DRS4 unit, and the time stamps are extracted from the pulse shapes using the Gaussian fit for the Hamamatsu MCP-PMT and the constant-fraction fit for the Photek MCP-PMTs. To alleviate smearing of the TOF due to uncertainty in the transverse position of the electron beam, the times extracted from the two Photek MCP-PMTs are averaged to obtain a single value for the arrival time of the scintillation light.

Download English Version:

<https://daneshyari.com/en/article/8173127>

Download Persian Version:

<https://daneshyari.com/article/8173127>

[Daneshyari.com](https://daneshyari.com)