



Contents lists available at ScienceDirect

Journal of Oral and Maxillofacial Surgery, Medicine, and Pathology

journal homepage: www.elsevier.com/locate/jomsm

Technical note

A new way of evaluating the biomechanics of the mandible with freedom in three axes in space: Technical note

Josete Barbosa C. Meira^a, Higor Landgraf^b, Elio Hitoshi Shinohara^c, João Gualberto C. Luz^{b,*}, Rafael Yague Ballester^a

^a Department of Biomaterials and Oral Biology, School of Dentistry, University of São Paulo, São Paulo, SP, Brazil

^b Department of Oral and Maxillofacial Surgery, School of Dentistry, University of São Paulo, São Paulo, SP, Brazil

^c Graduate Program, Araçatuba Dental School, Universidade Estadual Paulista “Julio de Mesquita Filho”, SP, Brazil

ARTICLE INFO

Keywords:

Mandible
In vitro techniques
Apparatus and instruments
Elasticity

ABSTRACT

Objective: A biomechanical analysis of fixation devices to repair fractures or osteotomies of the mandible is carried out in hemi-mandibles fixed in the condylar process, the force is applied in the molar region and a single movement is allowed. This technical note presents a new setup for evaluating the biomechanics of the mandible with the following improvements: (1) providing freedom of mobility in three axes in the space; (2) applying forces in a way that closely replicates that of real cases; (3) capable of evaluating the fracture resistance and the stiffness and elastic recovery.

Method: A rigid metal support mounted on bearings was developed that allowed the movement and deformation of the mandible during load application to mimic its freedom of movement when in function. Steadying was only in the mandibular fossae and free in all other regions. Ten fresh sheep mandibles were subjected to testing of their rigidity and capacity for elastic recovery after a displacement of 0.75 mm.

Results: After three displacement cycles, the mean value of stiffness was 506 ± 64 N/mm, and the mandibles showed visco-elastic recovery.

Conclusion: This new apparatus and approach is promising for use in the evaluation of mandibular fixations.

1. Introduction

Laboratory studies for the biomechanical evaluation of fixation devices to repair fractures or following sagittal split osteotomy have greatly contributed to improvement of mandibular fixations. Thus, several means of fixation have been developed in terms of the types and number of plates [1,2] and the isolated use of screws [3–6]. Many studies are still researching ideal fixation methods.

The occurrence of mandibular flexure has been established and may be of clinical importance [7]. However, most studies have used models with a cantilever setup, in which one end of the specimen is held rigidly fixed and the load is applied at the other end. Comparative studies on these mechanical fixing methods have been carried out and characterized in hemi-mandibles that are fixed in the condylar process. Force is applied in the molar region until fracture [8–10]. Therefore, a single movement is allowed, and the effects are limited.

The purpose of this technical note is to present a new way of evaluating the biomechanics of the mandibles that provides freedom of movement in three axes in space and measures stiffness.

2. Methods

2.1. Preparing the sheep mandibles

Ten fresh mandibles were selected for this study from similar sheep with similar weight and ages and collected from the same abattoir. The mandibles were dissected with complete removal of soft tissues. The coronoid processes were removed to facilitate the positioning of the mandible. These were selected from a group of twenty by measuring the following distances using callipers: posterior border - mental foramen and lower border - head of the condyle. For storage, the mandibles were packed in polyethylene bags and kept in refrigeration at 20 °C for up to 5 h prior to the experiment.

Because sheep mandibles have fibrous articulation in the middle region of the symphysis, they received fixation with two screws in the anterior portion to the mental foramen. This fixation was executed according to the pattern of lag screw to maintain a rigid assembly of the two hemi-mandibles. Subsequently, acrylic resin was adapted over a sectioned tube of half-round (rigid polyvinyl chloride – PVC). This PVC

* Corresponding author at: Department of Oral and Maxillofacial Surgery, School of Dentistry, University of São Paulo, Av. Prof. Lineu Prestes, 2227, 05508-900, São Paulo, SP, Brazil.
E-mail address: jgcluz@usp.br (J.G.C. Luz).

<https://doi.org/10.1016/j.ajoms.2018.03.011>

Received 25 November 2016; Received in revised form 27 June 2017; Accepted 27 March 2018

2212-5558/ © 2018 Asian Association of Oral and Maxillofacial Surgeons. Published by Elsevier Ltd All rights reserved.

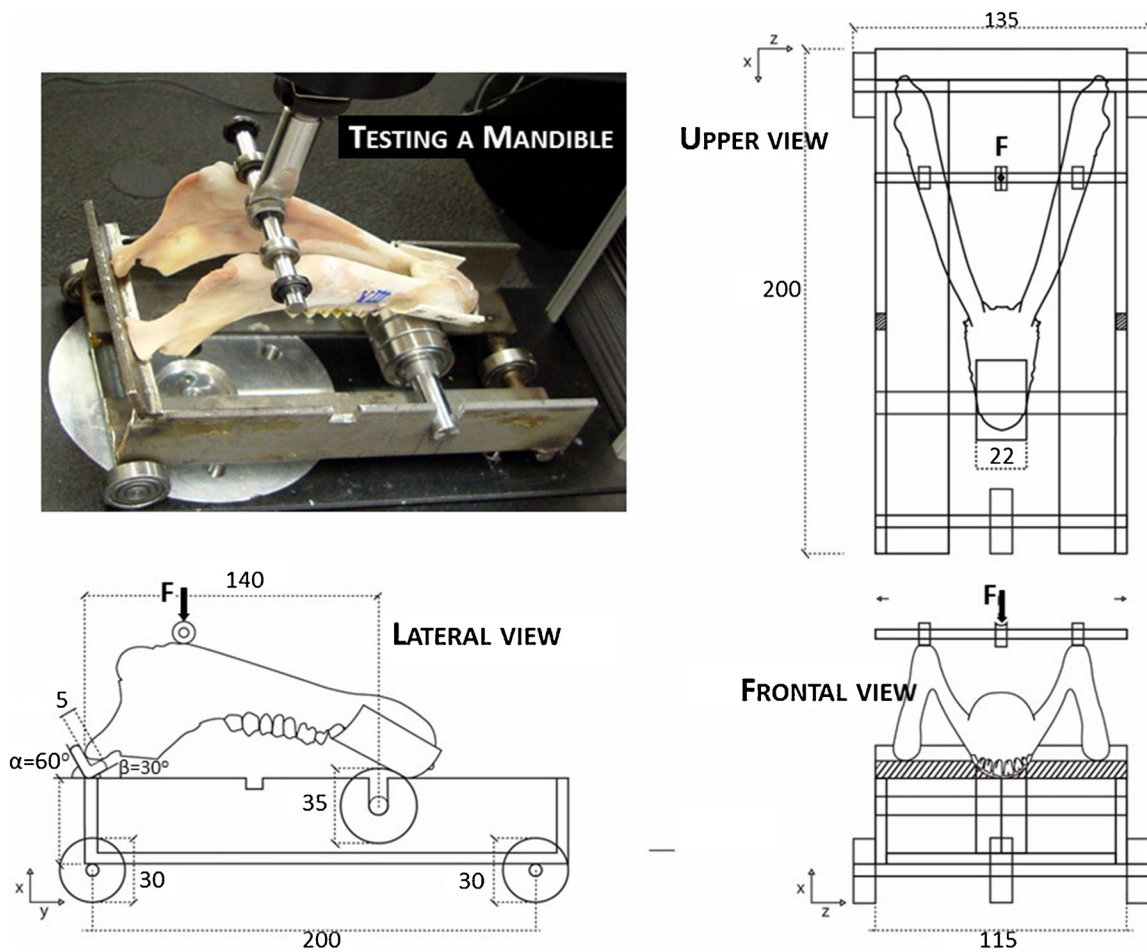


Fig. 1. Picture and the corresponding schematic drawing of a mandible assembled in the apparatus for testing.

base served as a sliding holder in each assay (Fig. 1) for the anterior region of the mandible. After correct positioning of the mandible and centralization of the apparatus on the universal testing machine, the mechanical testing was executed.

2.2. New device support

A rigid metal support mounted on bearings was developed to allow the movement of the whole mandible, while preserving the alignment of the load application point with the cross head of the testing machine throughout the test (Fig. 1). The load was applied on the central sliding bearing, which was mounted in a rigid metal bar with three sliding bearings. The two lateral sliding bearings were supported, stabilized and glued (acrylic resin, not represented in Fig. 1) in the left and right angles of the mandible, thus allowing the deformation of the mandible during load application by moving away or nearing the angles. The anterior region of the sheep mandibles was embedded in a PVC pipe cut into a half-round. This region was then supported over a rolling bearing to allow the deformation of the mandibles by increasing the angle between the body and the ramus to mimic the freedom of movement of a human mandible when in function. Both condyles were supported in a holder that mimicked the condylar fossa, which allowed only spinning. The mandible was free in all other regions. The positioning of the mandible in the apparatus occurred at three points of support: the condyles and the anterior region. The load application occurred bilaterally in the region between the mandibular body and angle, which is the area with the greatest muscle insertion, as represented by the region of the masseter muscle. The direction of the force applied was approximate to that of the masseter fibres.

2.3. Mechanical test

The mechanical test was performed in a universal testing machine, Instron 5565 (Illinois Tool Works Inc., Norwood, MA, US). The load and crosshead displacement data were recorded during the test, thus allowing the creation of a load versus displacement graph.

The mandibles were subjected to testing for rigidity in a non-destructive test. Three displacement cycles were applied at a rate of 0.07 mm/s for loading and 0.14 mm/s for unloading, with an interval of 120 s between each cycle. The first displacement was 0.25 mm, the second was 0.5 mm and the third was 0.75 mm. The waiting time for the mandible returns to the starting position was two minutes. The angular coefficient of the straight line, adjusted to the points corresponding to the load period of the last cycle, was adopted as a stiffness value in the curve load versus displacement. The formula $a = y/x$, where a = stiffness, y = load, and x = displacement, was adopted (Fig. 2). To calculate the mandibular stiffness, the third cycle was adopted as a standard because it had better uniformity in the graphic layout, possibly due to a better accommodation of the jaw on the metal apparatus. Fig. 2 shows the method used to calculate the stiffness of the mandible, and the results are shown in Fig. 3. A trend line was adjusted to the loading aspect of the register.

For the calculation of the horizontal displacement, rings were added with a metallic antenna in the bearings and a ruler was affixed in the support. The tips of the antennas moved as the displacement of the bearings that were located fixed in the angles of the mandibles. A camera was positioned to record the horizontal movement of the mandibular angles during the test, thus recording the horizontal displacement in millimeters.

Download English Version:

<https://daneshyari.com/en/article/8963624>

Download Persian Version:

<https://daneshyari.com/article/8963624>

[Daneshyari.com](https://daneshyari.com)